




Resolución mm		0.01	
Punto (Point)	Valor nominal mm	Error de medida μm	$U \pm (k=2)$ μm
	POSICIONES		
1	0.01	1.3	1.8
2	0.10	0.9	1.8
3	0.20	1.3	1.8
4	0.30	0.9	1.8
5	0.40	1.1	1.8
6	0.50	1.1	1.8
7	0.60	1.0	1.8
8	0.70	1.0	1.8
9	0.80	1.1	1.8
10	0.90	1.5	1.8
11	1.00	1.4	1.8

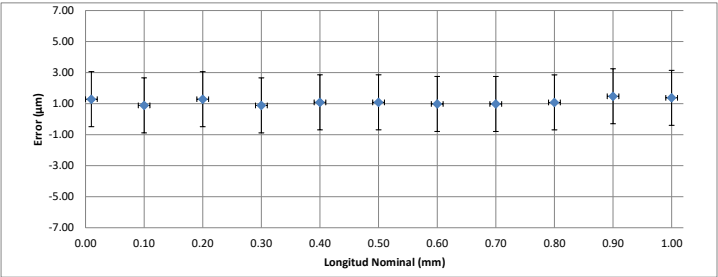

Resolución mm		0.1	
Punto (Point)	Valor nominal mm	Error de medida μm	$U \pm (k=2)$ μm
	POSICIONES		
1	0.10	0.9	2.4
2	1.00	1.9	2.4
3	2.00	3.9	2.4
4	3.00	1.4	2.4
5	4.00	1.4	2.4
6	5.00	1.4	2.4
7	6.00	1.1	2.4
8	7.00	1.1	2.4
9	8.00	1.3	2.4
10	9.00	0.9	2.4
11	10.00	1.0	2.4

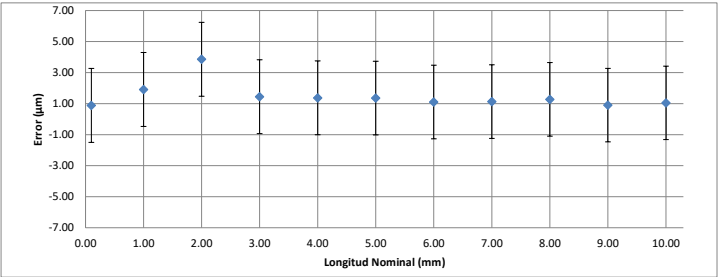

Resolución mm		1.0	
Punto (Point)	Valor nominal mm	Error de medida μm	U± (k=2) μm
	POSICIONES		
1	1.00	1.7	1.7
2	2.00	1.7	1.7
3	4.00	1.7	1.7
4	6.00	1.7	1.7
5	8.00	1.4	1.7
6	10.00	1.7	1.6
7	12.00	1.4	1.6
8	14.00	1.4	1.6
9	16.00	1.0	1.6
10	18.00	1.1	1.6
11	20.00	1.0	1.6

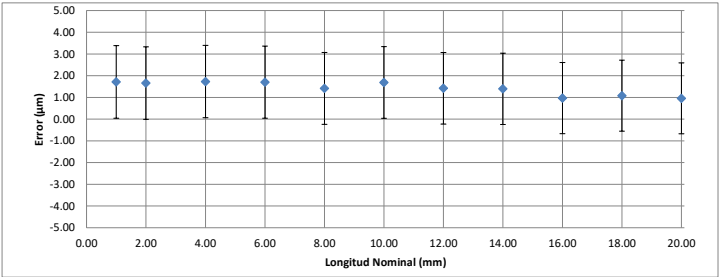

Condiciones del instrumento:
(Instrument conditions)

Sin comentarios.

Requerimientos del cliente:
(Customer requirements)

Sin requerimientos.