


Resultados de la calibración
(Results of calibration)

Punto (Point)	Valor nominal (Nominal value) mm	Error de indicación (Indication error) mm	Incertidumbre de medida (Measurement uncertainty) mm
1	2.500 0	-0.000 1	0.001 1
2	5.100 0	0.000 0	0.001 1
3	7.700 0	0.000 5	0.001 1
4	10.300 0	0.000 6	0.001 1
5	12.900 0	0.000 9	0.001 1
6	15.000 0	0.001 9	0.001 1
7	17.600 0	0.000 0	0.001 1
8	20.200 0	0.001 9	0.001 2
9	22.800 0	0.002 2	0.001 2
10	25.000 0	0.001 1	0.001 3

Fuerza de medición (Measuring force) N	Incertidumbre de medida (Measurement uncertainty) N
9.00	0.65

Variación del error de indicación (Indication error variation) mm	Incertidumbre de medida (Measurement uncertainty) mm
0.000 00	0.000 20

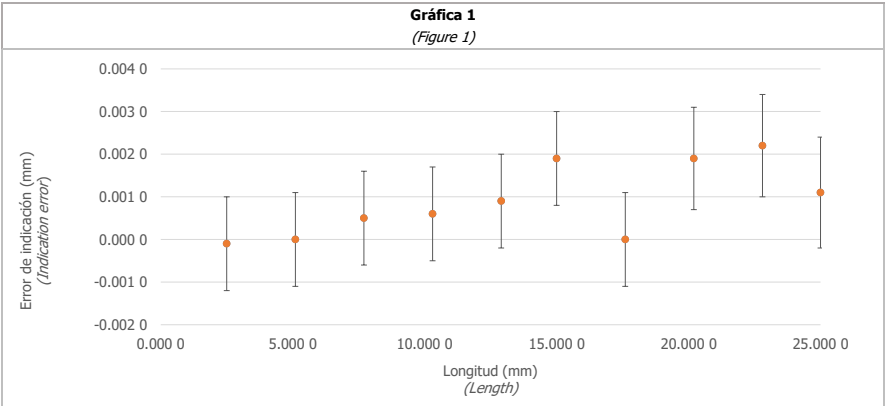

Condiciones del instrumento:
(Instrument conditions)

Sin comentarios

Requerimientos del cliente:
(Customer requirements)

Sin requerimientos.