


Resultados de la calibración:
(Calibration Results)

Magnitud:	Tensión	Tipo:	Directa	Unidad:	V	Medición	OUT	Resol. IBC:	0.01		
Patrón:	Fluke 8845A	Intervalo:	Desde:	3	Hasta:	30	Frec (Hz)	0			
Punto	Valor del IBC	Lecturas del Patrón					Error	k (95%)	U (95%)	Tolerancia Fabricante	D.C.
1	3	1	2	3	4	5					
1	3	3.00	3.00	3.00	3.00	3.00	0.0025	2.00	0.01	0.01	PASS
2	7.5	7.50	7.50	7.50	7.50	7.50	0.0027	2.00	0.01	0.01	PASS
3	15	15.00	15.00	15.00	15.00	15.00	0.0037	2.00	0.01	0.03	PASS
4	22.5	22.50	22.50	22.50	22.50	22.50	0.0037	2.00	0.01	0.04	PASS
5	27	27.01	27.01	27.01	27.01	27.01	-0.0061	2.00	0.01	0.05	PASS

Tolerancia de fabricante: $\pm(0.1\% \text{ Valor medido} + 0,010 \text{ mV})$ $\pm(0.1\% \text{ Valor medido} + 0,020 \text{ mV})$

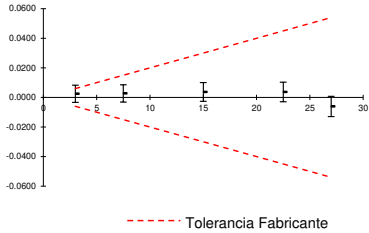

Magnitud:	Corriente	Tipo:	Directa	Unidad:	mA	Medición	OUT	Resol. IBC:	0.01		
Patron:	Fluke 8845A		Intervalo:	Desde:	7.2	Hasta:	72	Frec (Hz)	0		
Puntos	Valor IBC	Lecturas del Patrón					Error	k (95%)	U (95%)	Tolerancia Fabricante	D.C.
		1	2	3	4	5					
1	7.2	7.20	7.20	7.20	7.20	7.20	0.003	2.00	0.013	0.01	PASS
2	18	18.01	18.01	18.01	18.01	18.01	-0.010	2.00	0.030	0.04	PASS
3	30	29.97	29.97	29.97	29.97	29.97	0.027	2.00	0.043	0.06	PASS
4	54	53.99	53.99	53.99	53.99	53.99	0.007	2.00	0.069	0.11	PASS
5	64.8	64.78	64.78	64.78	64.78	64.78	0.016	2.00	0.081	0.13	PASS

Tolerancia de fabricante: $\pm(0.1\% \text{ Valor medido} + , 0,060 \text{ mV})$ $\pm(0.1\% \text{ Valor medido} + , 0,070 \text{ mV})$

