



Resultados de la calibración
(Results of calibration)

Punto (Point)	Valor nominal (Nominal Value) mm	Error de medida (Measurement Error) μm	U± (k=2) μm
	POSICIONES		
1	1.00	-0.92	1.5
2	2.00	-0.94	1.5
3	4.00	0.04	1.5
4	6.00	-0.98	1.5
5	8.00	-1.10	1.5
6	10.00	-0.43	1.5
7	12.00	-0.85	1.6
8	14.00	-0.87	1.6
9	16.00	-0.79	1.6
10	18.00	-1.01	1.6
11	20.00	-0.93	1.6

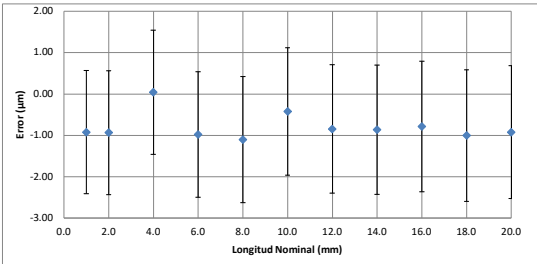


Resultados de la calibración
(Results of calibration)

Punto (Point)	Valor nominal (Nominal Value) mm	Error de medida (Measurement Error) μm	U ± (k=2) μm
	POSICIONES		
1	0.10	0.64	1.5
2	1.00	-0.35	1.5
3	2.00	-0.24	1.5
4	3.00	0.77	1.5
5	4.00	0.27	1.5
6	5.00	0.28	1.5
7	6.00	0.39	1.5
8	7.00	-0.10	1.5
9	8.00	-0.09	1.5
10	9.00	0.41	1.5
11	10.00	0.52	1.5

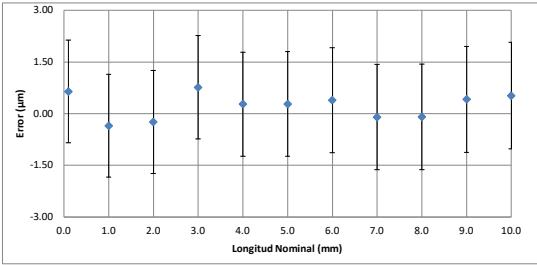

Resultados de la calibración
(Results of calibration)

Punto (Point)	Valor nominal (Nominal Value) mm	Error de medida (Measurement Error) µm	U± (k=2) µm
	POSICIONES		
1	0.01	-0.36	1.5
2	0.10	-0.36	1.5
3	0.20	-0.36	1.5
4	0.30	-0.36	1.5
5	0.40	-0.36	1.5
6	0.50	0.14	1.5
7	0.60	-0.35	1.5
8	0.70	0.15	1.5
9	0.80	-0.35	1.5
10	0.90	-0.85	1.5
11	1.00	0.15	1.5

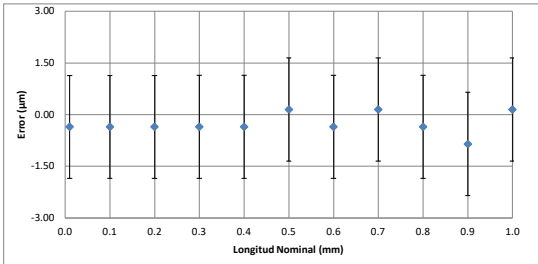

Condiciones del instrumento:
(Instrument conditions)

Sin comentarios.

Requerimientos del cliente:
(Customer requirements)

Sin requerimientos.