


Resultados de la calibración
(Results of calibration)

Punto (Point)	Valor nominal (Nominal Value) mm	Error de medida (Measurement Error) µm	U± (k=2) µm
	POSICIONES		
1	1.00	-1.65	1.6
2	5.00	-1.84	1.6
3	10.00	-1.48	1.6
4	15.00	-1.14	1.7
5	20.00	-0.80	1.7
6	25.00	-0.16	1.7
7	30.00	-0.16	1.8
8	35.00	-0.64	1.8
9	40.00	-0.73	1.8
10	45.00	-0.43	1.9
11	50.00	-0.55	1.9

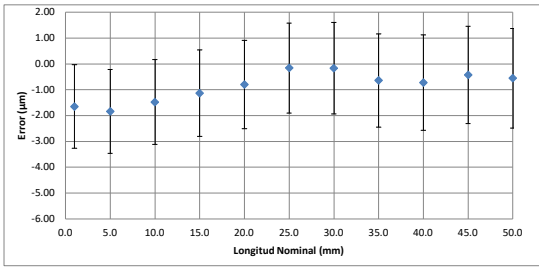

Condiciones del instrumento:
(Instrument conditions)

Sin comentarios.

Requerimientos del cliente:
(Customer requirements)

A prescripción del cliente, se documenta y aplica la frecuencia de calibración.