


Resultados de la calibración
(Results of calibration)

Punto (Point)	Valor nominal (Nominal Value) mm	Error de medida (Measurement Error) μm	$U\pm$ (k=2) μm
	POSICIONES		
1	1.00	-1.85	1.5
2	2.00	-1.84	1.5
3	4.00	-0.33	1.5
4	5.00	-0.42	1.5
5	10.00	-0.38	1.5
6	15.00	-0.44	1.6
7	20.00	0.80	1.6
8	22.00	1.32	1.6
9	24.10	0.43	1.6
10	24.82	2.44	1.7
11	25.00	1.44	1.7

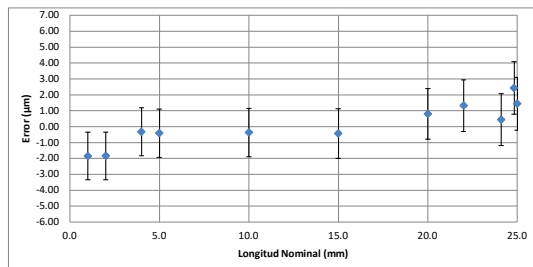

Condiciones del instrumento:
(Instrument conditions)

Sin comentarios.

Requerimientos del cliente:
(Customer requirements)

Sin requerimientos.