



Resultados de la calibración
(Results of calibration)

Punto (Point)	Valor nominal (Nominal Value) mm	Error de medida (Measurement Error) μm	$U \pm (k=2)$ μm
	POSICIONES		
1	1.00	0.58	1.5
2	2.00	0.06	1.5
3	4.00	0.94	1.5
4	6.00	0.92	1.5
5	8.00	0.90	1.5
6	10.00	0.37	1.5
7	12.00	0.35	1.6
8	14.00	0.93	1.6
9	16.00	0.91	1.6
10	18.00	1.19	1.6
11	20.00	0.97	1.6

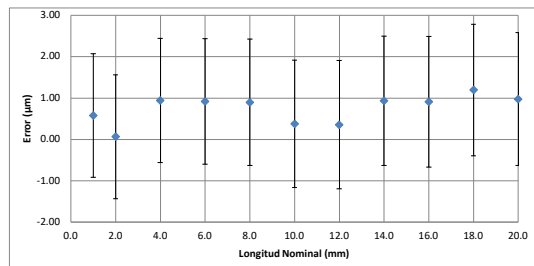


Resultados de la calibración
(Results of calibration)

Punto (Point)	Valor nominal (Nominal Value) mm	Error de medida (Measurement Error) μm	$U\pm$ (k=2) μm
	POSICIONES		
1	0.10	-0.86	1.5
2	1.00	-1.35	1.5
3	2.00	-0.84	1.5
4	3.00	-1.33	1.5
5	4.00	-0.93	1.5
6	5.00	-1.42	1.5
7	6.00	-1.41	1.5
8	7.00	-0.90	1.5
9	8.00	-1.39	1.5
10	9.00	-1.39	1.5
11	10.00	-1.38	1.5

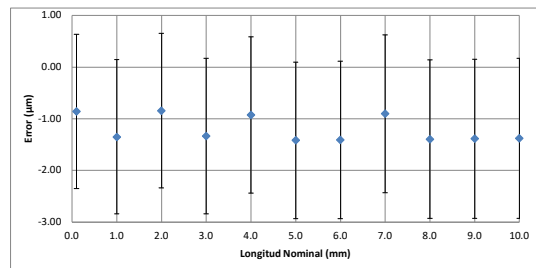

Resultados de la calibración
(Results of calibration)

Punto (Point)	Valor nominal (Nominal Value) mm	Error de medida (Measurement Error) μm	$U \pm (k=2)$ μm
	POSICIONES		
1	0.01	-0.36	1.5
2	0.10	0.14	1.5
3	0.20	-0.86	1.5
4	0.30	-0.86	1.5
5	0.40	-0.36	1.5
6	0.50	-0.86	1.5
7	0.60	-0.85	1.5
8	0.70	-0.85	1.5
9	0.80	-0.85	1.5
10	0.90	-0.85	1.5
11	1.00	-0.85	1.5

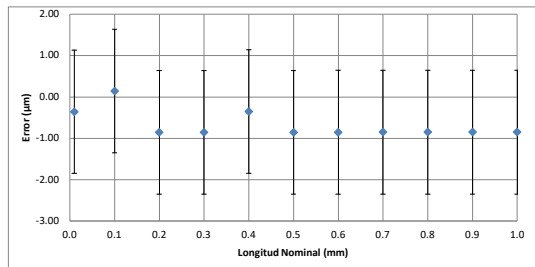

Condiciones del instrumento:
(Instrument conditions)

Sin comentarios.

Requerimientos del cliente:
(Customer requirements)

Sin requerimientos.