

Resultados de la calibración
(*Calibration results*)

Cota	Valor nominal (<i>Nominal value</i>)	Valor mínimo (<i>Minimal value</i>)	Valor máximo (<i>Maximum value</i>)	Promedio (<i>Average</i>)	Desviación estándar (<i>Standard deviation</i>)	Incertidumbre de medida (<i>Measurement uncertainty</i>)
	mm	mm	mm	mm	mm	mm
d	0.400	0.396 0	0.401 0	0.398 8	0.001 1	0.003 0
W (x)	0.600 0	0.582 0	0.608 0	0.595 8	0.007 0	0.003 2
W (y)	0.600 0	0.585 0	0.639 0	0.600 4	0.006 6	0.003 2

Figura 1.
(*Figure 1*)

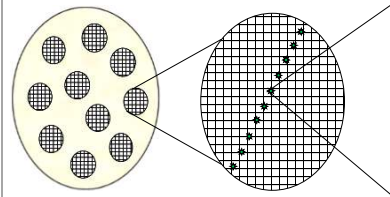


Figura 2.
(*Figure 2*)


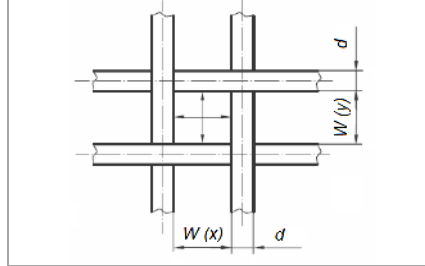


Figura 3.
(*Figure 3*)

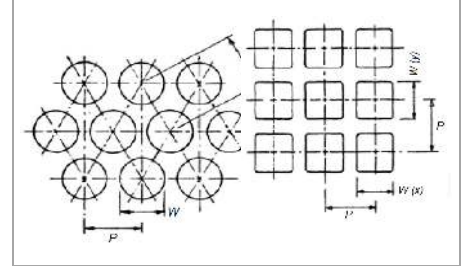

Condiciones del instrumento:
(*Instrument conditions*)

Sin comentarios

Requerimientos del cliente:
(*Customer requirements*)

Sin requerimientos.