



Resultados de la calibración (Calibration results)

Magnitud (Magnitude)	Temperatura "In" (Temperature "In")					Gráfica de resultado (Grafic of result)
Intervalo de medida (Measurement range)	-20 °C	a (to)	70 °C			
Resolución (Resolution)	0.1 °C					
Punto (Point)	Valor de referencia (Reference value)	Promedio IBC (Average)	Corrección (Correction)	Incertidumbre de medida (Measurement uncertainty)	#	°C
1	15.15	15.3	0.2	0.10		
2	20.19	20.4	0.2	0.10		
3	24.89	25.3	0.4	0.10		
4	29.98	30.4	0.4	0.10		
5	34.92	35.2	0.3	0.10		

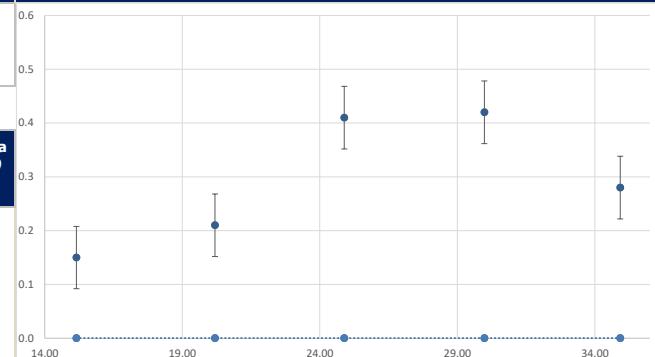

Magnitud (Magnitude)	Temperatura "Out" (Temperature "Out")					Gráfica de resultado (Grafic of result)
Intervalo de medida (Measurement range)	-50 °C	a (to)	70 °C			
Resolución (Resolution)	0.1 °C					
Punto (Point)	Valor de referencia (Reference value)	Promedio IBC (Average)	Sesgo instrumental (Instrumental bias)	Incertidumbre de medida (Measurement uncertainty)	#	°C
1	15.15	15.5	0.4	0.10		
2	20.19	20.5	0.3	0.10		
3	24.89	25.4	0.5	0.10		
4	29.98	30.4	0.4	0.10		
5	34.92	35.2	0.3	0.10		
14.00	15.5	0.00				
19.00	20.5	0.00				
24.00	25.4	0.00				
29.00	30.4	0.00				
34.00	35.2	0.00				

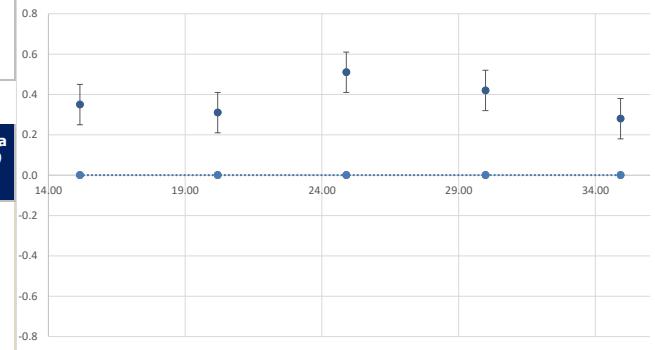

Condiciones del instrumento:
(Instrument conditions)

Sin comentarios.

Requerimientos del cliente:
(Customer requirements)

Sin requerimientos